



INSTRUCTIONS FOR USE

Product Name

Disposable Automatically Retractable Insulin Safety Syringe

Construction and specification

- The Construction includes barrel, piston, plunger, needle hub, needle, sealing ring, retractable member, end cap, protecting cap and end protecting cap
- Specification of syringe: 0.3ml 0.5ml 1ml
- Specification of needle: 0.25mm (31G), 0.3mm (30G), 0.33mm (29G), 0.36mm (28G), 0.4mm (27G)

Performance and features

- Sterile, Pyrogen free.
- Safety feature operates with one hand.
- Harmless to patient and medical staff once needle is retracted. (The needle can retract directly from the body.)
- The needle will remain sharp after puncturing the stopper on the medicine vial up to 3 times(fig 2).

Indications for use





The Disposable Automatically Retractable Insulin Safety Syringe is a sterile, disposable, automatically retractable safety syringe intended for subcutaneous injection of insulin into the body, while reducing the risk of sharps injuries and the potential for syringe reuse.

This syringe is designed for injection of insulin concentration type U-40 and U-100.






Instructions for use

Clinicians shall be familiar with the Instructions for use and be trained in the administration of clinical injections. The proper steps for use are as outlined below.

1. Peel open the package and remove the protective cap from the needle and from the plunger (fig 1).
2. Insert the needle into the medicine vial to draw medication into the barrel (fig 2).
3. Expel all air bubbles within the barrel of the syringe and then perform the injection. Inject slowly (fig 3).
4. Depress the plunger all of the way within the barrel and when injection is completed, the needle will automatically retract (fig 4).



Ver. IFU-I A5
Effective date: 2022.3.4

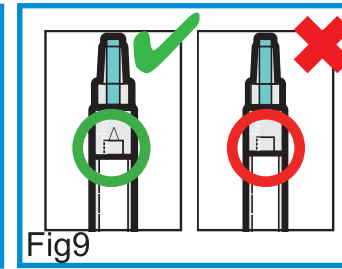

Cautions

1. Please read the "Instructions for use" section before use.
2. Do not use if package is damaged or protective cap is detached.
3. The syringes are sterile until removed from their protective packaging. Single use only.
4. Carefully check if there is a shaft in the front of the plunger before use. Do not use the product if there is no shaft (fig 9).
5. Do not use excessive force when drawing the liquid into the syringe as this may unseat the "O" ring or cause needle non-retraction (fig 5).
6. Do not push plunger over the "warning" line before injection (fig 6).
7. Inject slowly. Injecting too quickly may unseat the "O" ring and cause failure to retract (fig 5).
8. Safety features can only be activated when the medicine or fluid is fully discharged. (Needle cannot be automatically retracted if medicine or fluid is not fully discharged) (fig 7).
9. If the needle cannot be automatically retracted after medicine or fluid has been fully discharged, please pull back the plunger until the needle is inside the barrel (fig 8).
10. Dispose of the syringe in an appropriate sharps container per protocol of your institution.
11. Federal law restricts this device to sale by or on the order of a physician.

Symbol

1. Single use only. 

2. Sterilized using ethylene oxide.

STERILE EO



Expiry date 3 years

Storage

To be protected from moisture and heat. Should be kept indoors, without corrosive gas, dry, well ventilated and clean.

Manufacturer

Shantou Wealy Medical Instrument Co., Ltd.
North Jinhuan Road (near Qishan Mid-School), Shantou, China
Postcode:515064
Telephone:+86 754 8212 1967
Fax: +86 754 8212 1370